Figure E1

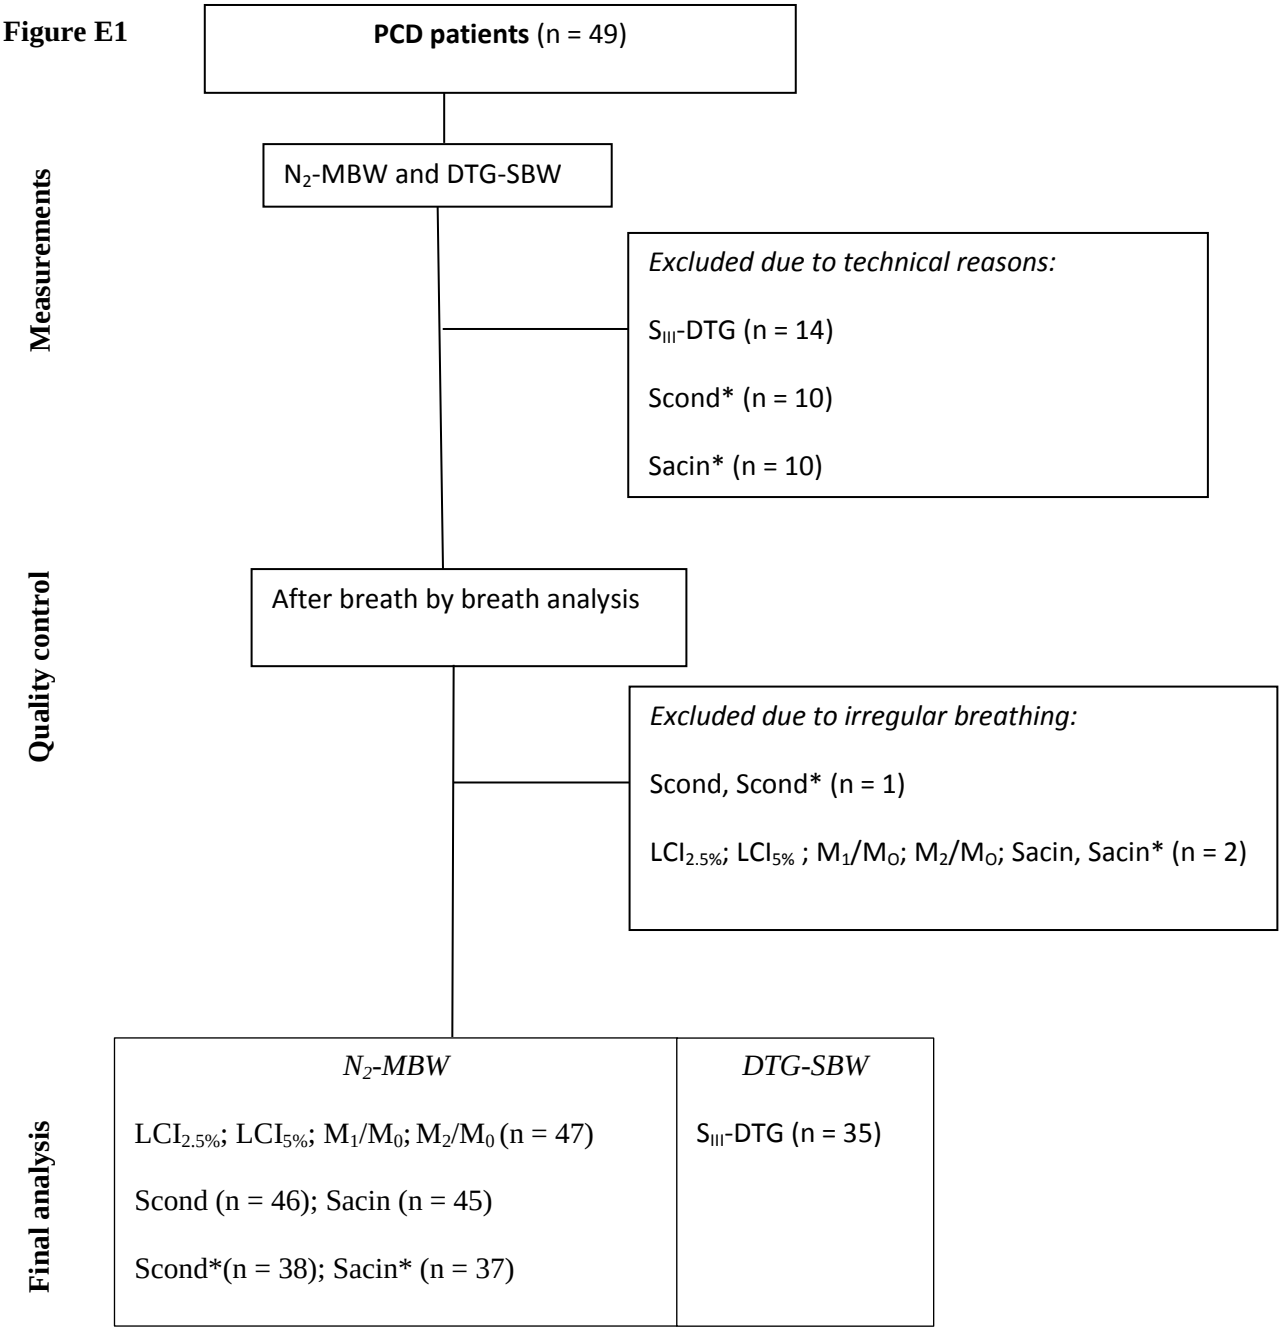
PCD patients (n = 49)
Measurements
N2-MBW and DTG-SBW
Excluded due to technical reasons:
SIII-DTG (n = 14)
Scond* (n = 10)
Sacin* (n = 10)
Quality control
After breath by breath analysis
Excluded due to irregular breathing:
Scond, Scond* (n = 1)
LCI2.5%; LCI5% ; M1/M0; M2/M0; Sacin, Sacin* (n = 2)
Final analysis
N2-MBW
LCI2.5%; LCI5%; M1/M0; M2/M0 (n = 47)
Scond (n = 46); Sacin (n = 45)
Scond*(n = 38); Sacin* (n = 37)
DTG-SBW
SIII-DTG (n = 35)